



**Whitehall Manufacturing®**  
Manufacturer of Healthcare and Rehabilitation Products since 1946

Division of  
Acorn Engineering Company®



A MEMBER OF



## Lo-Boy Whirlpools

Use



# L Series 90 Gallon Stationary Whirlpool

## L-90-S



L-90-S

**Whitehall L-90-S Stationary Whirlpool** is recommended to facilitate hydrotherapy of extremities, hip and back area and allows spaces for exercising.

**Whirlpool Tank** is 60"L x 24"W x 18"D and is seamless welded construction, fabricated from heavy gauge, type 304 stainless steel, polished to a satin finish. Tank rim is reinforced with a concealed stainless steel rod. Tank bottom is seamless, coved (rounded) design for effective cleaning. Tank is also provided with an extended stainless steel skirt flush to the floor line to conceal internal drain piping. A 2" Combination Drain and Overflow, and a Filler Spout are provided.

**Turbine Raising and Lowering Device** permits adjustment of desired height and direction of water agitation towards the area of the body during Whirlpool use. It is spring balanced and provided with a locking device.

**Turbine Assembly** is equipped with Underwriters Laboratory listed 1/2 HP jet pump motor protected with an ABS plastic shell, automatic thermal overload protector, and lifetime-sealed bearings. All parts contacting the water are stainless steel, chrome plated brass or bronze.

**Thermometer** is provided with a dual scale, adjustable calibration, and a stem inserts into a retainer to prevent rattle during whirlpool agitation.

### GUIDE SPECIFICATIONS

Provide Whitehall Stationary Whirlpool (specify model number and options) with a 90-gallon capacity, 60"L x 24"W x 18"D. Whirlpool shall be fabricated from heavy gauge, type 304 stainless steel. Construction shall be seamless welded and exposed surfaces shall be polished to satin finish. Tank shall have a reinforced rim and shall be fitted with a stainless steel skirt flush to the floor line. Bottom of tank shall be a seamless, rounded coved design. Provide a 2" combination drain and overflow, and a filler spout. Provide a turbine assembly with raising and lowering device which functions as an agitator and permits adjustment of desired height, direction of water agitation, and can be locked into place. Turbine assembly shall be UL listed 1/2 HP jet pump motor with automatic thermal overload protector and lifetime-sealed bearings. Provide a thermometer with a stem retainer to prevent rattle when whirlpool is in operation.

Please visit [www.whitehallmfg.com](http://www.whitehallmfg.com)  
for most current specifications.



Whitehall Mfg. • P.O. Box 3527 • City of Industry, CA 91744 • (800) 591-9280 • (626) 968-6681

L-90-S

REV: 07/02/2024



**Whitehall Manufacturing®**  
Manufacturer of Healthcare and Rehabilitation Products since 1946

## Lo-Boy Whirlpools

### MODEL NUMBER AND OPTION SELECTIONS

#### Series

☒ L Lo-Boy Series

#### Capacity

☒ -90 Gallons

#### Type

☒ -S Stationary Whirlpool

#### Turbine Electrical Requirements

☐ 115VAC / 50Hz ☐ 115VAC / 60Hz

☐ 230VAC / 50Hz ☐ 230VAC / 60Hz

Country of Use \_\_\_\_\_

#### For Mixing Valve:

Refer to supplemental MXT15-OTG and DU-1 sheet for details.

#### Suffix Options (See Whirlpool Options Section for Details)

- ☐ -AS3 Adjustable Suspension Seat
- ☐ -EG Enviro-Glaze® Color Powder Coating - Specify Color: <https://www.whitehallmfg.com/enviro-glaze>
- ☐ -GFI Ground Fault Interrupter
- ☐ -HR Head Rest, Adjustable
- ☐ -LOGO Applied Logos: Team, Facility, Company Logo
- ☐ -RS Reclining Seat
- ☐ -SDO Separate Drain Overflow Assembly
- ☐ -TTS2 Tank Top Seat

#### ELECTRIC REQUIREMENTS:



Amps: 6.9/6.2 Hertz: 50/60  
Volts: 115 GFI Receptacle

#### ELECTRIC REQUIREMENTS:

Amps: 3.5/3.1 Hertz: 50/60  
Volts: 230 GFI Receptacle

Certified per US & Canadian  
Medical Standards; UL  
60601-1 & CSA C22.2 No.  
601.1

Certified per  
European Standards;  
IEC 60601-1

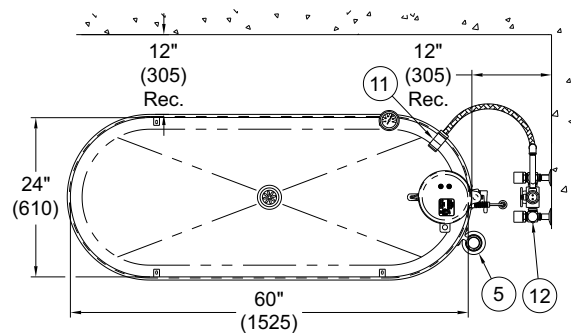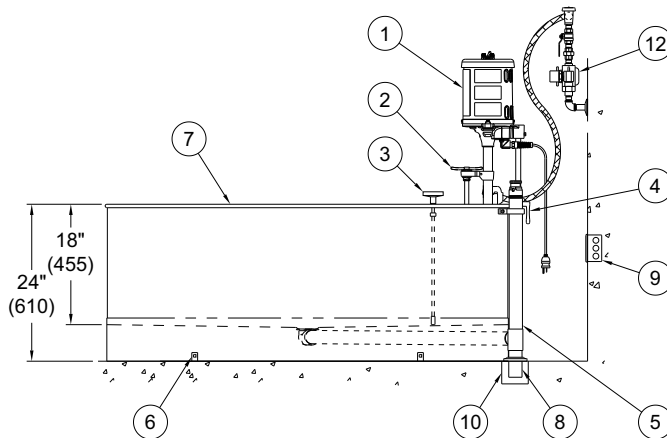

STATIONARY L-90-S SERIES WHIRLPOOL

#### NOTES:

- |                                      |                                          |                                            |
|--------------------------------------|------------------------------------------|--------------------------------------------|
| 1. 1/2 HP Jet Pump Motor             | 5. Combination Drain & Overflow Assembly | 9. 3 Pole GFI Receptacle by Others         |
| 2. Variable Pressure Control         |                                          | 10. Floor Drain by Others                  |
| 3. Thermometer                       | 6. "L" Brackets - (4) Four Each          | 11. Filler Spout                           |
| 4. Turbine Raising & Lowering Device | 7. Stainless Steel Tank                  | 12. Mixing Valve, Shown For Reference Only |
|                                      | 8. 2" O.D. x 5" Tailpiece                |                                            |

WARNING: Cancer and Reproductive Harm - www.P65Warnings.ca.gov

All dimensions are nominal and subject to manufacturer's change without notice. Whitehall assumes no responsibility for use of void or superseded data. © Whitehall Manufacturing, Member of Morris Group International. Please visit [www.whitehallmfg.com](http://www.whitehallmfg.com) for most current specifications.

#### SELECTION SUMMARY & APPROVAL FOR MANUFACTURING

Model Number & Options \_\_\_\_\_ Quantity \_\_\_\_\_  
Company \_\_\_\_\_ Date \_\_\_\_\_  
Contact \_\_\_\_\_ Title \_\_\_\_\_  
Approval for Manufacturing/Signature \_\_\_\_\_

Whitehall Mfg. • P.O. Box 3527 • City of Industry, CA 91744 • (800) 591-9280 • (626) 968-6681

**L-90-S**

REV: 07/02/2024